

# Identification of istihadhah blood color using TCS3200 color sensor with Multilayer Perceptron (MLP) method

**Syukrotus Sa'diati<sup>1\*</sup>, Heni Sumarti<sup>1</sup>, and Edi Daenuri Anwar<sup>1</sup>**

<sup>1</sup>Department of Physics, Faculty of Science and Technology, Universitas Islam Negeri Walisongo Semarang, Indonesia

\*Corresponding author's e-mail: syukrotus@gmail.com

## ABSTRACT

One of the natures of women, including menstruation, namely the discharge of blood from the vagina periodically and has a certain cycle. However, this cycle can experience disturbances, in Islam it is referred to as istihadloh. Women who are experiencing istihadloh are called mustahadloh. One of the mustahadloh categories is Mu'tadah Ghairu Mumayyizah, namely women who have recently bled but cannot distinguish between strong and weak blood. This study aims to distinguish between menstrual blood and istihadloh based on its color. The research method was carried out by designing and manufacturing the TCS3200 color sensor tool based on Arduino Uno with RGB value output results. The average RGB value of istihadloh blood is R 71.6, G 83.7 and B 55.2. While the average RGB values for menstrual blood color are R 143.3, G 176.6 and B 79.3. The results of the classification accuracy using the MLP method in differentiating menstrual blood and istihadloh based on color using the TCS3200 color sensor are 96.7%.

### Keywords:

Istihadloh, TCS3200 Sensor, RGB.

## Introduction

In Islam, particularly within Shafi'i jurisprudence (Fiqh Shafi'iyyah), there are three types of blood that may exit the female reproductive organ: menstrual blood (haidh), postpartum bleeding (nifas), and istihadhah blood (al-Bajuri). According to Bujairimi 'ala al-Khatib by Sulaiman bin Muhammad, menstruation linguistically means "to flow," while terminologically it refers to natural blood that exits a woman's vagina during a healthy state (not due to illness), unrelated to childbirth (nifas), and occurring at specific times. Imam Shafi'i categorized menstrual blood into five colors: black, red, reddish-gold, yellow, and turbid. Meanwhile, Imam Hanafi recognized six types: black, red, yellow, greenish, and soil-like in color (Nuruddin, 2018). There are cases of green menstrual blood, typically found in individuals suffering from malnutrition (Saribanon, 2016).

According to Shahih Fiqh Sunnah by Abu Malik Kamal bin as-Sayyid Salim, istihadhah is defined as blood that flows outside the menstrual or postpartum period, caused by a ruptured vein, and is typically fresh, continuous blood (Nailatus Sa'adah, 2020). A woman experiencing istihadhah is called a mustahadhah. Some women are unable to distinguish between menstrual and istihadhah blood when bleeding occurs, perceiving them as the same. Such women fall under the category of Mu'tadah Ghairu Mumayyizah (Barakah A., 2018).

In medical science, only two types of female reproductive bleeding are recognized: menstrual and postpartum. There is no term equivalent to istihadhah. Medically, menstruation results from the shedding of the uterine lining, composed of blood and tissue, not triggered by egg fertilization, and it occurs regularly in healthy women (Abdullah, 2019). Medically, istihadhah may be classified as pathological menstruation or a menstrual disorder, although this does not address its classification under Islamic law (Asyikin Y, et al., 2015). Clinically, it is known as menorrhagia (Mahadi, 2018), which is influenced by various factors such as stress, fatigue, medication side effects, contraceptive use, or medical conditions like endometriosis, polyps, myomas, and cervical cancer (Fuadah, 2017).

Menorrhagia refers to excessive menstrual bleeding lasting several consecutive cycles, with blood volume reaching or exceeding 80 mL per cycle. As such, it is considered a significant health

concern for women (M. K. Oehler, 2003). In Islam, women experiencing istihadhah are still required to perform ibadah mahdhah (ritual worship) such as prayer, reciting the Qur'an, fasting, and pilgrimage, as they are still considered ritually pure (tahir) and not in a state of hadath (impurity) (Syah, 2017).

From a medical perspective, the color of menstrual and istihadhah blood is essentially the same, but variations occur due to external factors. Menstrual blood changes color depending on how long it remains in the vagina, typically darkening from red to brown or black due to exposure to acidity (Auliawati, 2009). However, understanding of istihadhah remains limited since only a subset of women experience it. Therefore, there is a need for a tool that can identify istihadhah blood to support both health monitoring and religious practices.

Based on its characteristics, istihadhah blood can be identified through indicators such as odor, viscosity, and color. Thus, potential detection tools include odor sensors, viscosity sensors, and color sensors. In this study, the distinguishing indicator used is color. The most suitable tool for identifying color differences between menstrual and istihadhah blood is the TCS3200 color sensor. This sensor is commonly used for color detection applications, such as in Simamora's study (2017), which successfully identified meat freshness levels based on color using the TCS3200 sensor. This sensor can respond to differences in red levels that indicate freshness in meat. The TCS3200 uses microcontroller technology, with one of the most widely developed platforms being Arduino Uno, a versatile and accessible tool for educational and practical applications (Mintoro, 2018).

The visible spectrum refers to the full range of colors perceivable by the human eye and represents a depiction of visible light. Visible light is a form of electromagnetic radiation and is part of the electromagnetic spectrum. Electromagnetic radiation travels in waves with varying wavelengths and frequencies. The wavelength of the visible spectrum is measured in nanometers ( $10^{-9}$  m), and frequency in terahertz ( $10^{12}$  Hz). The visible colors, from shortest to longest wavelength, are violet, indigo, blue, green, yellow, orange, and red. Each color occupies a specific wavelength range within the 400–700 nm spectrum (Ryan Johnson, 2021). Rainbows visually represent the continuous frequency range of visible light (Gaikwad, 2019).

The TCS3200 color sensor is a chip that converts light from a specific color into a frequency output. It consists of two main components: an array of photodiodes arranged in parallel and an inverter section. The TCS3200 uses photodiodes with filters for red, green, and blue (RGB) as well as photodiodes without filters. Each section of the sensor operates at an 8-bit scale (Artha, 2012). Arduino Uno is an open-source electronics prototyping platform based on a microcontroller chip. It is designed to simplify the application of electronics across various fields (Setiadi, 2019). "Uno" means "one" in Italian. This microcontroller board is based on the Atmega328 chip, featuring 14 digital I/O pins (6 of which support PWM output), 6 analog inputs, a 16 MHz quartz crystal oscillator, USB connection, power jack, ICSP header, and a reset button. To use the microcontroller, the Arduino Uno board can be connected to a DC adapter or battery using a USB or AC power cable (Zulkarnain, Ramadhan, & Anwar, 2019).


Multilayer Perceptron (MLP) is a classification algorithm in Artificial Neural Networks (ANN) used to analyze datasets. MLP is a powerful class of nonlinear statistical models composed of multiple layers of nodes in a directed graph, where each layer is fully connected to the next (Castro et al., 2017). This study addresses the issue that many women remain unable to differentiate between menstrual and istihadhah blood based on color, which is crucial for religious obligations. The research aims to determine the average RGB values of menstrual and istihadhah blood, and to evaluate the classification accuracy of the TCS3200 color sensor using the MLP method. The study's significance lies in its potential contribution to researchers, healthcare professionals, and institutions by offering a non-invasive method to aid in distinguishing these two types of blood.

## **Methods**

This research employed the Research and Development (R&D) method, resulting in the creation of a functional product. The research stages included tool design, device assembly, data grouping, and data identification. The tools and materials used in this study are Arduino Uno, LCD 6x12, Jumper Cables, TCS3200 Color Sensor, IC 7805, Resistors, Battery, Hole-type PCB, ON/OFF Switch, WEKA Software and Arduino IDE Software.

### *Research Procedure*

The experimental procedure involved the following stages: tool design, calibration, data collection, and data classification (Figure 1). Tool testing included both calibration and accuracy testing. Calibration was performed by comparing the RGB values of a red-colored object to similar RGB values obtained in previous studies. The calibrated RGB values were then used for accuracy evaluation.

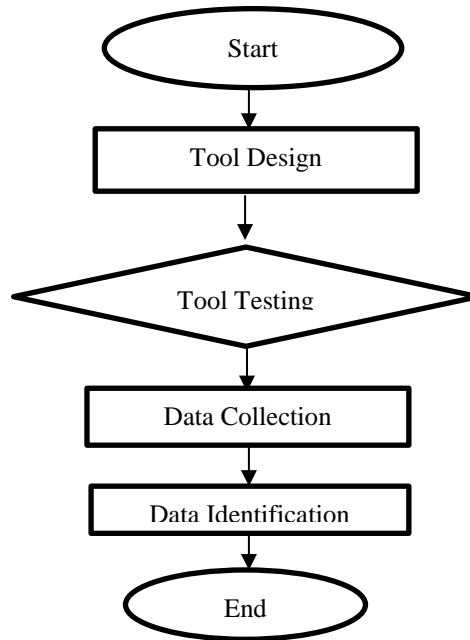

**Figure 1.** Research Procedure Diagram


To calculate measurement error and accuracy, the following formulas were used:

$$Error = \frac{\text{Measured Value} - \text{Standard Value}}{\text{Standard Value}} \times 100\% \quad (1)$$

$$Accuracy = 100\% - error \quad (2)$$

### *Tool Design*


Figure 2 show design of the Istihadhah Blood Identification Tool Using TCS3200 Color Sensor

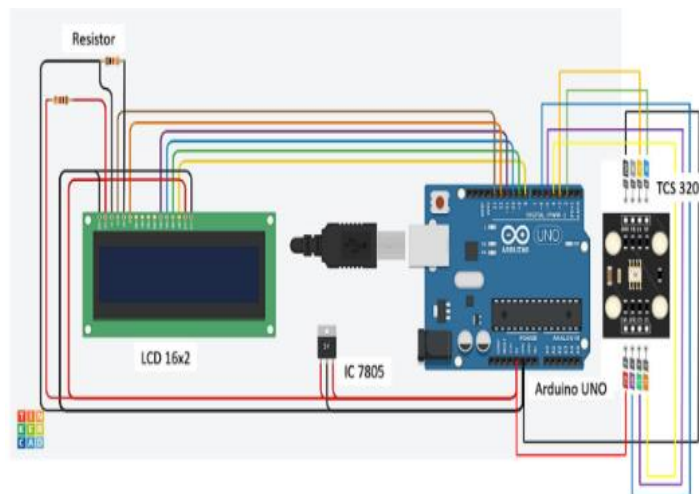

**Figure 2.** Design of the Istihadhah Blood Identification Tool Using TCS3200 Color Sensor

### *Sample Data Collection Method*

Blood samples were collected from the surface of sanitary pads (Figure 3). The surface area of the blood stain on the pad had to match the detection area of the color sensor. If the stained area was smaller than the sensor's detection area, the sample was considered invalid. Valid samples were scanned using the TCS3200 color sensor, and the resulting RGB values were displayed on the LCD screen. The sensor irradiated a 4×4 cm area, corresponding to its detection range, to ensure consistency during data collection.

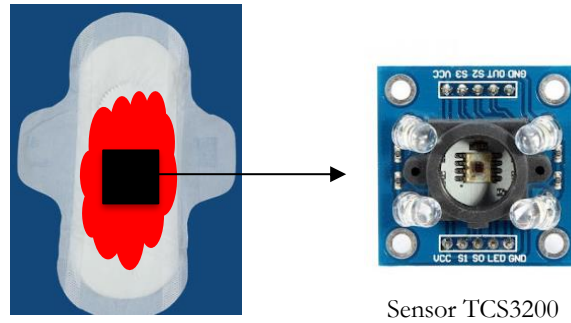

**Figure 3.** Blood Sample Collection Method

#### *Data Analysis Technique*

The collected RGB data series from each sample were compiled in Microsoft Excel and converted into CSV format before classification using the WEKA software. The classification matrix in WEKA includes: TP (True Positive), FP (False Positive), TN (True Negative), and FN (False Negative). Performance metrics such as accuracy, sensitivity, and specificity were calculated using the following formulas:

$$Accuracy = \frac{TP + TN}{TP + FP + FN + TN} \times 100\% \quad (3)$$

$$Sensitivity = \frac{TP}{TP + FN} \times 100\% \quad (4)$$

$$Specificity = \frac{TN}{TN + FP} \times 100\% \quad (5)$$


## **Result and Discussions**

#### *TCS3200 Color Sensor Prototype for Istihadloh Blood Identification*

Results obtained in this research include a color identification tool prototype for differentiating menstruation and istihadloh using the TCS3200 color sensor (figure 4). This prototype is designed as electronic hardware including the TCS3200 color sensor connected to Arduino Uno, then connected through Arduino IDE software for sensor program settings to obtain data. Color detection with the TCS3200 sensor works when photodiodes receive input signals, then current continues from photodiodes and is converted to square signals.

#### *Calibration*

Calibration was performed on red-colored paper samples. This was done to adjust red color range values on the istihadloh blood color identification tool prototype with color range values performed on plain red-colored paper. Testing in this research was performed at a 4.0 cm distance from objects, where at this distance, TCS3200 sensor illumination corresponds to object cross-sectional areas with dimensions between 3.5×3.5 cm to 5×5.5 cm<sup>2</sup> (Table 1).

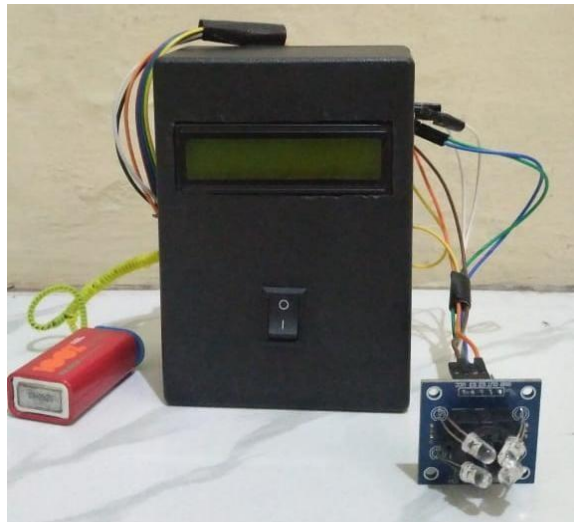

**Figure 4.** Menstrual and Istihadloh Blood Color Identification Tool Prototype

**Table 1.** Average Red Color Values

RGB	Value 1	Value 2	Value 3	Value 4	Value 5	Average
<b>R</b>	138	131	130	136	137	134.4
<b>G</b>	183	184	182	187	182	183.6
<b>B</b>	137	140	144	143	143	141.4

#### *Accuracy Testing*

Accuracy testing was performed to determine error levels occurring in data classification (Sampurno & Thoriq, 2016). Accuracy testing includes error percentages is shown in Table 2.

**Table 2.** Accuracy and Error Percentages

RGB	Standard Value	Measured Value	Error	Accuracy
<b>R</b>	133.0	134.4	1.1%	98.9%
<b>G</b>	178.0	183.6	3.1%	96.9%
<b>B</b>	146.0	141.4	3.2%	96.8%
<b>Average</b>	<b>152.3</b>	<b>153.1</b>	<b>2.5%</b>	<b>97.5%</b>


#### *Sample Data Collection*

Sample data was obtained from 10 women experiencing menstruation and 10 women experiencing istihadloh, with each sample data collected three times over three consecutive days when discharged blood was red. Thus, 60 data points were obtained with 30 menstruation data and 30 istihadloh data respectively. Average color values for menstrual blood and istihadloh have been presented in graphs 5, 6, and 7. These graphs show comparisons and classifications of menstrual blood and istihadloh color values across red, green, and blue periods.


Graphs 5, 6, and 7 show that average istihadloh blood color is lower than average menstrual blood color, making istihadloh blood color lighter or more faded than menstrual blood with clearer red color. These three graphs demonstrate that menstrual blood and istihadloh blood have different RGB range values and can be classified based on color. Based on graphs, istihadloh blood color appears pinkish-red, while menstrual blood color appears red.

#### *Data Classification*


TP (True Positive) indicates correct data for istihadloh, FP (False Positive) indicates error data for istihadloh. Meanwhile, TN (True Negative) indicates correct data for menstruation and FN (False Negative) indicates error data for menstruation. Therefore, data accuracy percentage, data sensitivity, and data specificity of 96.7% were obtained (Table 3).

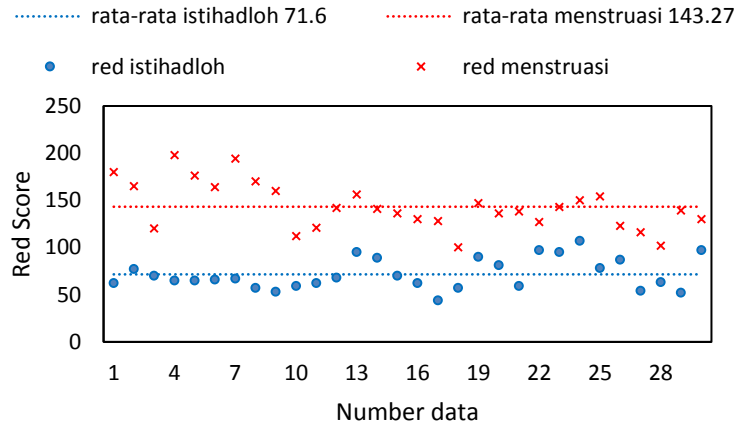

**Figure 5.** Comparison of Average Menstrual and Istihadloh Blood Color Values for Red Period

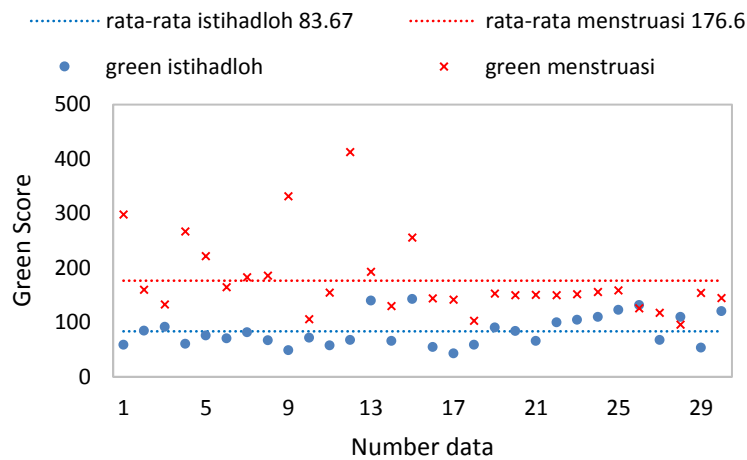

**Figure 6.** Comparison of Average Menstrual and Istihadloh Blood Color Values for Green Period

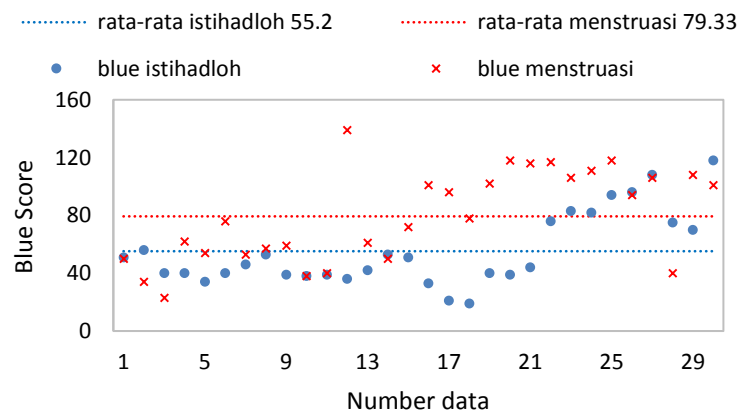

**Figure 7.** Comparison of Average Menstrual and Istihadloh Blood Color Values for Blue Period

**Table 3.** Results of TP, FP, TN, FN, Accuracy Percentage, Sensitivity and Specificity

TP	FP	TN	FN	Accuracy	Sensitivity	Specificity
29	1	29	1	96.7%	96.7%	96.7%

### Discussion

Medical condition diagnoses experienced during menstrual disorders include urinary tract infections, ectopic pregnancy, and irritable bowel syndrome. Additionally, endometriosis and uterine fibroids can

cause heavy bleeding and chronic pain. To confirm these diagnoses, examinations can be performed through Ultrasonography and Sonohisteriography, which are imaging techniques often used to detect specific conditions possibly caused by menstrual disorders (Resources, 2022). According to fiqh scholars, differences between menstruation and istihadloh, besides temporal aspects, can be seen from emergence location. Menstrual blood emerges from the uterine tip, while istihadloh blood emerges from the cervical opening or lowest uterine part (Nuroniayah, 2019). Non-invasive istihadloh blood identification tool development has not been discussed, as istihadloh blood identification is only based on menstrual period calculations. Innovation in creating istihadloh blood identification tools is expected to become a media development facilitating Muslim women when encountering abnormal menstrual cycles.

This prototype uses the TCS3200 color sensor based on Arduino Uno displaying output in Red, Green, and Blue (RGB) values. Testing was performed on sample data then averaged. Average values for menstrual blood and istihadloh show differences between these two blood colors. Based on Table 4, average RGB values for menstrual blood color are higher compared to average RGB values for istihadloh blood color. There is a comparison between TCS3200 color sensor Red Green Blue (RGB) output values for dark-colored objects versus light-colored objects. Darker object colors result in higher RGB values on the TCS3200 color sensor, conversely, lighter object colors result in lower RGB values on the sensor (Ratnawati & Vivianti, 2018). Based on research results, istihadloh blood has lighter red color compared to menstrual blood.

**Table 4.** Average RGB Value Ranges for Menstrual Blood and Istihadloh

<b>RGB</b>	<b>Menstruation</b>	<b>Istihadloh</b>
R	143.3	71.6
G	176.6	83.7
B	79.3	55.2

Previous theory explained that menstrual blood experiences considerable settling time in the uterus, making its color darker, while istihadloh blood emerges outside the menstrual cycle, so blood does not experience settling time and has lighter color (Dan Brennan, 2021). Additionally, fiqh scholars provide calculation methods for determining menstrual blood and istihadloh status: 'adah method and tamyiz method. The 'adah method calculates habits or customs from menstrual periods, while the tamyiz method calculates blood status by observing strength and weakness of emerging blood. If emerging blood is strong, it is considered menstruation; if emerging blood is categorically weak, it is considered istihadloh (Nuroniayah, 2019). According to scholars, blood strength and weakness are observed from color aspects, having very concentrated colors. If emerging blood has concentrated red color, it is considered strong blood. Meanwhile, if emerging blood has light red color, it is considered weak blood (Barakah A., 2018).

Based on the above theory, this corresponds to TCS3200 color sensor RGB values for object brightness and darkness. Thus, it can be stated that lighter blood will be read as weak blood and categorized as istihadloh blood. Istihadloh blood color is pink, as istihadloh blood RGB ranges fall between pink and red colors (Appendix 1). However, it should be noted that during measurement using the TCS3200 color sensor, small possibilities exist for light distraction, affecting resulting RGB values. This research uses average RGB values obtained based on menstrual blood and istihadloh RGB color range results. This was done to focus on one number for easier data analysis reading.

Based on graphs 5, 6, and 7, menstrual blood and istihadloh RGB values are stable only for R values; for G and B values in menstruation and istihadloh data, they intersect. This occurs because each RGB value has optimum distances. Research by Athifa and Rachmat (2019) shows that TCS3200 color sensor RGB values have optimum distances during object illumination, resulting in fluctuative distances during object illumination. Based on this research, resulting data shows R values can detect colors well up to 6.5 cm distance. G and B values can detect colors well up to 3.5 cm distance. G and B values become fluctuative after 3.5 cm distance. Meanwhile, in this research, object illumination was performed at 4 cm distance, causing G and B values to experience fluctuation resulting in G and B values in menstrual blood intersecting with istihadloh blood.

Menstrual blood color and istihadloh blood color classification was determined through WEKA software using the Multilayer Perceptron (MLP) method with 96.7% accuracy results. One menstruation data was categorized as istihadloh data (data sequence 49) and one istihadloh data was categorized as menstruation data (data sequence 40). This shows that occasionally menstrual blood range values can be low and istihadloh blood range values can be high.

However, in this research, blood RGB value measurements were not pure because blood absorbed into pads made blood redness fade. Additionally, wet or dry blood conditions already attached to pads caused by pad absorption of blood were considered, as this would affect RGB values. Therefore, blood illumination was standardized, performed when pads were not too wet or had already absorbed. In this research, RGB value readings for pads were ignored.

WEKA detection or identification errors were caused by similar color ranges. Menstruation RGB values (data sequence 49) of 100, 103, 78 tended more toward istihadloh RGB value range categories. Conversely, istihadloh RGB values (data sequence 40) of 107, 110, 82 tended more toward menstruation RGB value range categories. Additionally, surrounding light can affect RGB value readings on objects.

## **Conclusion**

Average RGB values for istihadloh blood color were **R** 71.6; **G** 83.7 and **B** 55.2. Meanwhile, menstrual blood color ranges were **R** 143.3; **G** 176.6 and **B** 79.3. Istihadloh blood RGB values show lighter red color compared to menstrual blood with darker red color. This occurs because istihadloh blood does not experience prolonged settling like menstrual blood. Classification accuracy using the MLP method in differentiating menstrual blood and istihadloh based on color using the TCS3200 color sensor achieved 96.7%. The istihadloh blood identification tool should be developed by adding aroma sensors and humidity sensors to become a more adequate health tool innovation. This research should be used as a reference for future research.

## **Acknowledgments**

We would like to thank Department of Physics, Universitas Islam Negeri Walisongo Semarang for providing the necessary facilities and resources for this work.

## **Conflicts of interest**

The authors affirm that they have no conflicts of interest.

## **References**

- 2002M, L.-P. (2008). *Sumber rujukan: Permasalahan wanita Uyunul Masail Linnisa'*. Kediri: Lirboyo.
- A Islamiy, F. F. (2020). *Faktor-Faktor yang Mempengaruhi Siklus Menstruasi pada Remaja Putri Tingkat III*. Tulungagung: STIKES Utama Abdi Husada .
- Abdullah, M. K. (2019). Blood Women in erspective of Fiqh Syafi'iyah and Medical Science. *Britain International of Humanities and Social Sciences Journal*.
- Afrilia. (2017). *Aplikasi Rancangan Acak Lengkap 1 Faktor*. Kalimantan Timur: [http://kaltim.litbang.pertanian.go.id/ind/index.php?option=com\\_content&view=article&id=899&Itemid=59](http://kaltim.litbang.pertanian.go.id/ind/index.php?option=com_content&view=article&id=899&Itemid=59).
- al-Bajuri, S. I. (n.d.). *Al-Bajuri 'Ala Ibni Qasim al-Ghazi, Juz I*. Surabaya: Nurul Huda.
- Aryani, R. (2010). Kesehatan Remaja Problem dan Solusinya. *Salemba Medika*.
- Athifa, S. F., & Rachmat , H. H. (2019). Evaluasi Karakteristik Deteksi Warna RGB Sensor TCS3200 Berdasarkan Jarak Dan Dimensi. *JETri*, 105-120.
- Auliawati, I. (2009). *Pandangan Imam Malik dan medis tentang perbedaan haid dengan istihadah*. Surabaya: UIN Sunan Ampel.
- Barakah, A. (2018). Istihadhah Dan problematikanya dalam kehidupan praktis masyarakat. *CENDEKIA : Jurnal Studi Keislaman*, 1(1).



- Baratloo, A., Hosseini, M., Negida, A., & Ashal, G. E. (2015). Part 1: Simple Definition and Calculation of Accuracy, Sensitivity and Specificity. *Emerg (Tehran)*, 48-49.
- Bernard, S. A. (2012). Linking Strategy, Business, and Technology EA3 An Introduction to Enterprise Architecture. *United States: Bloomington*.
- Campbell. (1999). *Biologi jilid I*. Jakarta: Erlangga.
- Dadang. (2009, Februari 18). *Dosen ITS Ciptakan Alat Sensor Aroma*. Retrieved from ITS News: <https://www.its.ac.id/news/2009/02/18/dosen-its-ciptakan-alat-sensor-aroma/>
- Dahri, N. (2012). Reproduksi Perempuan Dalam Perspektif Islam (Tinjauan terhadap Haid, Nifas, dan Istihadah). *Marwah (Jurnal Perempuan Agama dan Jender)*.
- Dan Brennan, M. (2021, June 05). What to Know About the Color of Period Blood. *Women's Health*, p. 1.
- Dr. Muhammad Yusro, M. D. (2019). Sensor Dan Transduser (Teori dan Aplikasi). Jakarta: Fakultas Teknik UNJ.
- Evin Dwi Prayuni, A. I. (2018). Therapy for Irregular Menstruation with Acupuncture. *Journal of Vocational Health Studies*.
- Fikriyah Hasanah, M. S. (2018). Pengaruh Intensitas Spektrum Cahaya Warna Merah Dan Hijau Terhadap Perkecambahan Dan Fotosintesis Kacang Hijau (*Vigna Radiata L.*). *Gravity Vol.4 No.2*.
- Fuadah, d. N. (2017, Oktober 17). *Tanya Dokter*. Retrieved from Alodokter: <https://www.alodokter.com/komunitas/topic/haidistidhadah>
- Gaikwad, D. A. (2019). Colour Spectrum. *Granthalayah*.
- Gharrafi. (2009). Menstrual Cycle Patterns of Collage Students in Gorgan-Northeast of Iran : Identify its Association with Sociodemographic Factors. *Erciye Tip Dergisi*, (pp. 331-338).
- Handoyo, S. &. (2002). Analisa Manajemen Sistem Informasi Koperasi Simpan Pinjam Berbasis Multi User Dengan Metode RnD. *Jurnal Publikasi Manajemen Informatika*, (1), 6-17.
- Hennegan J, N. S. (2020). Measuring menstrual hygiene experience: development and validation of the Menstrual Practice Needs Scale. In Soroti Uganda.
- Heyi Yang, B. Z. (2012). Proteomic Analysis of Menstrual Blood. *PMC Journal List*.
- Jalaluddin, M. H. (2020). *Sistem Penyortiran Buah Apel Menggunakan Sensor TCS3200 Dan Mikrokontroler Berbasis Android*. Medan: Universitas Sumatera Utara.
- Johar, M. A. (2014). Metode Penelitian Teknik Informatika. . *Deepublish*.
- Linden, D. L. (2002). Handbook of Batteries 3 Ed. Amerika Serikat.
- M. K. Oehler, M. C. (2003). Menorrhagia: an update, *Acta Obstetricia et Gynecologica Scandinavica. Obstetrics & Gynaecology*.
- Mahadi, S. A. (2018). Pengurusan Istihadah Menurut Fiqh Islam dan Perubatan. *Asian People Journal*.
- Mintoro, S. (2018). Pemanfaatan Teknologi dan Informasi Mikrokontroler. *Seminar Nasional Teknologi dan Bisnis 2018* (p. 1). Bandar Lampung: IIB DARMAJAYA.
- Musarofah, S. M. (2020). Reproduction Health Based on Various Kinds of Women's Blood in Serat Piwulang Estri and Risalah Al-Mahid: Philological and Comparative Studies. . *Journal of Social Transformation and Regional Development*, 2(3), 56-62.
- N. Ismail, M. C. (2016). Kefahaman Pelajar Terhadap Fiqh Thaharah:(Permasalahan Darah Wanita): Tinjauan di UITM Cawangan Perlis. In *3rd International Conference on Arabic Studies and Islamic Civilization, Akademi pengajian Islam Kontemporari (ACIS)*.
- N. Saribanon, M. T. (2016). *Haid dan Kesehatan Menurut Ajaran Islam*. Jakarta Selatan: Sekolah Pascasarjana Universitas Nasional.
- Nailatus Sa'adah, A. A. (2020). Hukum Seputar Darah perempuan Dalam Islam. *Martabat: Jurnal Perempuan dan Anak*.
- Na'imah, F. U. (2016). Tinjauan Madzhab Shafi'i dan Madzhab Hanbali Tentang Haid yang Terputus- Putus Serta Akibat Hukumnya. *Al-'Adalah : Jurnal Syari'ah dan Hukum Islam*.
- Nor Asyikin Y, N. D. (2015). Knowledge of and attitudes towards of menstrual disorders adults in north-eastern state of Peninsular Malaysia. *Malaysian Family Physician*, 9.
- Nugroho, S., & Rianto, A. (2021). Sistem Deteksi Penyiraaan Otomatis Berdasar Perubahan Warna Kandungan Kadar Air Daun Jamur Kuping Berbasis IoT (Internet of Things). *E-Prosiding Seminar Nasional Hasil Penelitian Lembaga Penelitian dan Pengabdian Masyarakat* . Semarang: Universitas Semarrang.

- Nuroniayah, W. (2019). *Fikih Menstruasi Menghapus Mitos-Mitos dalam Menstrual Taboo*. Depok: PT Rajawali Buana Pusaka.
- Nuruddin, S. M. (2018). *Cara Wanita menghadapi haid, nifas, dan istihadhah menurut Al-Qur'an dan Hadits*. Jakarta Selatan: Al-Kautsar Prima.
- Papib Handoko, Y. F. (2013). Pengaruh Spektrum Cahaya Tampak Terhadap Laju Fotosintesis Tanaman Air Hydrilla Verticillata. Seminar Nasional X Pendidikan Biologi Fkip UNS. *Jurnal.Fkip.Uns.Ac.Id*, 10(3), 15-147.
- Patil. (2013). Menstrual Pattern among Adolescent Girl In Rural Area Of Bijapur. *Al Ameen J med Sci*.
- Pratama, M. A., Shidiq, A. F., Rahmanto, Y., & Surahman, A. (2021). Perancangan Sistem Kendali Alat Elektronik Rumah Tangga. *JTIKOM*.
- Proverawati, A. (2009.). Menarche Menstruasi Pertama Penuh Makna. *Yogyakarta : Mulia Medika*.
- Ratnawati, D., & Vivianti. (2018). Alat Pendeteksi Warna Menggunakan Sensor Warna TCS3200 dan Arduino Nano. *Prosiding Seminar Nasional Vokasi Indonesia*, (pp. 167-170).
- Resources, C.-1. S. (2022). *Menstrual Dis-orders*. Retrieved from Mount Sinai: <https://www.mountsinai.org/health-library/report/menstrual-disorders>
- Rihardini, T. (2019). Mengenali Ketidakaturan Siklus Menstruasi untuk Mendeteksi Gangguan Kesehatan Reproduksi pada Remaja di Kelurahan Gunung Anyar Tambak Surabaya. *SNHRP-II : Seminar Nasional Hasil Riset dan Pengabdian, Ke-II* (pp. 266-274). Surabaya: UNIPA Surabaya.
- Rosen, D. (2022, Maret 21). *What does your period blood colour mean?* Retrieved from Livi: <https://www.livi.co.uk/your-health/what-does-your-period-blood-colour-mean/>
- Ryan Johnson, T. Z. (2021, 10 21). *Study.com*. Retrieved from The Color Spectrum: Colors of Visible Light and Wavelengths: <https://study.com/learn/lesson/color-spectrum-visible-light-colors.html>
- Sabiq, S. (2013). *Fiqih sunnah 4 / Sayyid Sabiq ; Penerjemah: Abu Syaqqina, Abu Aulia Rahma*. Jakarta: Tinta Abadi Gemilang.
- Salmon Charles Siahaan, F. A. (2021). Gangguan Menstruasi dan Penyebabnya. *UC*.
- Sampurno, R. M., & Thoriq, A. (2016). Klasifikasi Tutupan Lahan Menggunakan Citra Landsat 8 Operasional Land Imaginer (OLI) di Kabupaten Sumedang. *Jurnal Teknotan*, 61-70.
- Saputra, H. A. (2015). Pemahaman Tentang Nifas dan Istihadah: Studi Kasus Ibu-Ibu Jama'ah Muslimat Yayasan Masjid Darussalam Tropodo Sidoarjo. *Justitia Islamica*.
- Setiadi, T. (2019, 12 11). M.Kom. Semarang, Jawa Tengah, Indonesia.
- Sigit Nugroho, P. (2008). Rancangan Percobaan. . *Bengkulu: UNIB Press*.
- Suci Damayanti, A. A. (2020). Problematika Istihadhoh Dalam Persepsi Wanita. *Al-Iman: Jurnal Keislaman dan Kemasyarakatan*.
- Sugiyono. (2016). Metode Penelitian Kuantitatif, Kualitatif dan R&D. *Bandung: PT Alfabet*.
- Sundayani, D., Witanti, W., Sabrina, P. N., & Priatna, S. (2020). Peranan Civitas Akademika dalam Revolusi Industri 4.0. *Seminar Nasional Informatika dan Aplikasinya (SNIA 19)*. Jawa Barat: Universitas Jenderal Achmad Yani .
- Swasty, W. (2010). A-Z Warna Interior Rumah Tinggal . *Griya Kreasi*.
- Swedia, E. R. (2010). *Algoritma Transformasi Ruang Warna*. Depok, Jakarta: Universitas Gunadharma.
- Syah, I. J. (2017). Mengenal Menstruasi Dalam Perspektif Imam Syafi'i. *Akademika*, 53-54.
- Syauqi, M. I. (2022, Oktober 23). *Thaharah: Cara Bersuci bagi Pengidap Besar dan istihadhah*. Retrieved from Nu Online: <https://islam.nu.or.id/thaharah/cara-bersuci-bagi-pengidap-besar-dan-istihadhah-7m4iZ>
- Tan, P. S. (2006). Introduction to Data Mining. *Boston: Pearson Education*.
- Tirtasari, N. L. (2017). Uji Kalibrasi (Ketidakpastian Pengukuran) Neraca Analitik di Laboratorium Biologi FMIPA UNNES. *Indonesian Journal of Chemical Science*.
- Wantania, J. J. (2016). Pendarahan Uterus Abnormal- Menoragia pada Remaja. *Junal Biomedik (JBM)*, 135-142.
- Zwinkels, J. (2015). Light, Electromagnetic Spectrum. In *Encyclopedia of Color Science and Technology* (pp. 1-8). Canada: National Research Council Canada.